

# Calibrating Unit

## New Standard Solution Report

|                         |                       |              |              |
|-------------------------|-----------------------|--------------|--------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C | Serial No.:  | ARXA-0069    |
| Location:               | MARLBORO TWP. POLICE  |              |              |
| Calibration File No.:   | 01000                 | Calib. Date: | 06/01/2022   |
| Certification File No.: | 01001                 | Cert. No.:   | 00049        |
| Linearity File No.:     | 01002                 | Cert. Date:  | 06/01/2022   |
| Solution File No.:      | 01003                 | Lin. Date:   | 06/01/2022   |
| Sequential File No.:    | 01003                 | Soln. Date:  | 06/01/2022   |
|                         |                       | File Date:   | 06/01/2022   |
| Calibrating Unit:       | WET                   | Model No.:   | CU-34        |
| Control Solution %:     | 0.100%                | Serial No.:  | DDXC S3-0162 |
| Solution Control Lot:   | 21270                 | Expires:     | 07/21/2023   |
|                         |                       | Bottle No.:  | 1123         |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 15:23D |                |                     |
| Control 1 EC      | 0.101% | 15:24D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.100% | 15:24D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:24D |                |                     |
| Control 2 EC      | 0.100% | 15:25D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 15:25D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:26D |                |                     |
| Control 3 EC      | 0.100% | 15:26D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.101% | 15:26D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:27D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

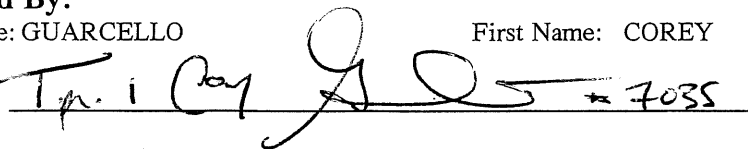
Temperature Probe Serial Number: DDUJ P2 - 066 (B)

**Changed By:**

Last Name: GUARCELLO

First Name: COREY

MI: R.

Signature: 

Badge No.: 7035

Date: 06/01/2022