

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0069
Location: MARLBORO TWP. POLICE
Calibration File No.: 00657 Calib. Date: 02/02/2017 Calib. No.: 00034
Certification File No.: 00658 Cert. Date: 02/02/2017 Cert. No.: 00025
Linearity File No.: 00659 Lin. Date: 02/02/2017 Lin. No.: 00029
Solution File No.: 00676 Soln. Date: 07/11/2017 Soln. No.: 00164
Sequential File No.: 00676 File Date: 07/11/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0162
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 1073

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:12D		
Control 1 EC	0.100%	08:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:13D		
Control 2 EC	0.100%	08:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:14D		
Control 3 EC	0.099%	08:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LOYER

First Name: JOHN

MI: B

Signature: _____

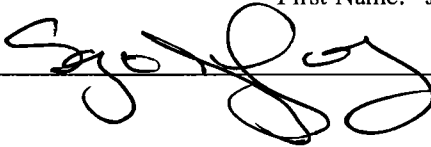

Badge No.: 057

Date: 07/11/2017

