

## ALCOTEST 9510 PARAMETER REPORT

### Equipment

Serial No.: ARMH-0009  
Firmware: 8326739 1.5  
WinCE application: 8326738 2.9  
Configuration: 8326737 3.10

Date: 02/04/2025  
Time: 11:39:35

### Parameter

min. blow time	5.0	s
min. breath volume for females of age 60+	1.2	L
min. breath volume for all other	1.5	L
min. blow flow	4.5	L/min
plateau detection limit	4	%
plateau detection start conc.	70	microgram/L
neg. flow detection (part. vacuum)	10.0	hPa
neg. flow detection sensitivity	10	
cal. gas abort volume	0.4	L
result-to-zero limit	0.0050	%BAC
ambient air check limit	0.0049	%BAC
interference det. d-criterion limit abs.	38	microgram/L
interference det. d-criterion limit rel.	10.0	%
interference det. t-criterion limit abs.	8	microgram/L
interference det. t-criterion limit rel.	2.1	%
IR CO2 offset	10	microgram/L
IR H2O offset	4	microgram/L
EC H2O offset	0	microgram/L
Value-based EC aging comp. on/off (1/0)	0	
Time-based EC aging comp. on/off (1/0)	1	
Time-based EC aging comp. per month	0.2	%
Time-based EC aging comp. maximum	3.0	%
EC fatigue comp. max. sum	15000	
EC fatigue comp. factor	50	
EC fatigue comp. minutes	180	
mouth alc. mark limit	500	
mouth alc. lower limit	30	
mouth alc. slope	6	
mouth alc. zero limit	50	
mouth alc. max. neg. sum	6	
mouth alc. max. 2nd derivative	35	

**ALCOTEST 9510 CERTIFICATION REPORT - WET ADJUST (PART I)**  
**Marlboro Township**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0009  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Wet Adjust Record**

Wet Adjust File No.: 213 Wet Adjust Date: 02/04/2025 Wet Adjust No.: 8  
Wet Adjust Time: 12:18:45

Concentration: 0.100 %  
Adjusting Unit: X-Cal 2000 Adj. Unit Ser. No.: ARRD-0003 Adj. Unit Exp.: 10/03/2025  
Solution Lot No.: 23240 Soln. Bottle No.: 236 Adjust Soln. Exp.: 06/28/2025

Preadjust Simulator Temp.: 34.00 degree C  
Postadjust Simulator Temp.: 34.00 degree C

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Waldrop - First Name: Robert MI: W Badge No.: 8256

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.



Signed:

Date: 02/04/2025

ID: 52

**ALCOTEST 9510 CERTIFICATION REPORT - DRY ADJUST (PART II)**  
**Marlboro Township**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0009  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Dry Adjust Record**

Dry Adjust File No.: 214 Dry Adjust Date: 02/04/2025 Dry Adjust No.: 8  
Dry Adjust Time: 12:47:55

Concentration: 0.100 %  
Dry Gas Lot No.: 302-402448282 Adjust Gas Exp.: 05/20/2025  
Barom. Model No.: Mensor CPG2300 Barom. Serial No.: 41001RDG Barom. Cert. Exp.: 09/26/2025  
Pre-adjust Amb. Pressure: 1009 hPa Post-adjust Amb. Pressure: 1009 hPa

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Waldrop - First Name: Robert MI: W Badge No.: 8256

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.



Signed:

Date: 02/04/2025

ID: 52

**ALCOTEST 9510 CERTIFICATION REPORT - LINEARITY (PART III)**  
**Marlboro Township**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0009  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Linearity Record**

Linearity File No.: 215 Lin. Date: 02/04/2025 Lin. No.: 8

0.040% Dry Gas Lot No.: 302-402488140 Adjust. Gas Exp.: 07/15/2025  
0.080% Dry Gas Lot No.: 302-402477282 Adjust. Gas Exp.: 06/24/2025  
0.160% Dry Gas Lot No.: 302-402486005 Adjust. Gas Exp.: 07/13/2025  
0.300% Dry Gas Lot No.: 302-402488144 Adjust. Gas Exp.: 07/15/2025

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	13:19:08		*TEST PASSED*
Control .04 Test 1 EC	0.039	13:19:46	1010	*TEST PASSED*
Control .04 Test 1 IR	0.039	13:19:46	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:20:51		*TEST PASSED*
Control .04 Test 2 EC	0.039	13:21:06	1010	*TEST PASSED*
Control .04 Test 2 IR	0.040	13:21:06	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:23:15		*TEST PASSED*
Control .08 Test 3 EC	0.078	13:23:53	1010	*TEST PASSED*
Control .08 Test 3 IR	0.080	13:23:53	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:25:05		*TEST PASSED*
Control .08 Test 4 EC	0.079	13:25:20	1010	*TEST PASSED*
Control .08 Test 4 IR	0.081	13:25:20	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:27:50		*TEST PASSED*
Control .16 Test 5 EC	0.153	13:28:26	1010	*TEST PASSED*
Control .16 Test 5 IR	0.159	13:28:26	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:29:41		*TEST PASSED*
Control .16 Test 6 EC	0.156	13:29:54	1010	*TEST PASSED*
Control .16 Test 6 IR	0.160	13:29:54	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:37:28		*TEST PASSED*
Control .30 Test 7 EC	0.285	13:38:05	1010	*TEST PASSED*
Control .30 Test 7 IR	0.297	13:38:05	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:39:35		*TEST PASSED*
Control .30 Test 8 EC	0.288	13:39:48	1010	*TEST PASSED*
Control .30 Test 8 IR	0.299	13:39:48	1010	*TEST PASSED*
Ambient Air Blank	0.000	13:40:25		*TEST PASSED*

**Result**

**All tests within acceptable tolerance.**

**Coordinator**

Last Name: Waldrop - First Name: Robert MI: W Badge No.: 8256

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.



Signed:

Date: 02/04/2025

ID: 52

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 1**  
**Marlboro Township**  
**SERIAL NUMBER: ARMH-0009**

**Equipment**

Inst. Model No.:	ALCOTEST 9510	Serial No.:	ARMH-0009	WinCE:	8326738 2.9
Firmware:	8326739 1.5	Config.:	8326737 3.10	Cyl1 Install No.:	3
Cyl1 Install File No.:	206	Cyl1 Install Date:	12/23/2024		

**Control Tests (0.100%)**

Installation Inlet:	#1 (Upper)	Post test active Cyl.:	#2 (Lower)
Dry Gas Lot No.:	302-403035121	Dry Gas Lot Exp.:	05/02/2027

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	13:43:19		*TEST PASSED*
Control Test 1			1029	*TEST PASSED*
EC Result	0.097	13:44:07		*TEST PASSED*
IR Result	0.101	13:44:07		*TEST PASSED*
Ambient Air Blank	0.000	13:45:18		*TEST PASSED*
Control Test 2			1029	*TEST PASSED*
EC Result	0.097	13:45:44		*TEST PASSED*
IR Result	0.101	13:45:44		*TEST PASSED*
Ambient Air Blank	0.000	13:46:55		*TEST PASSED*
Control Test 3			1029	*TEST PASSED*
EC Result	0.097	13:47:21		*TEST PASSED*
IR Result	0.101	13:47:21		*TEST PASSED*
Ambient Air Blank	0.000	13:47:49		*TEST PASSED*

**Result**

**All tests within acceptable tolerance.**

**Coordinator**

Last Name: Waldrop -                      First Name: Robert                      MI: W    Badge No.: 8256

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*TR Waldrop #8256*

Signed:

Date: 12/23/2024

ID: 52

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 2**  
**Marlboro Township**  
**SERIAL NUMBER: ARMH-0009**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0009  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
Cyl2 Install File No.: 172 Cyl2 Install Date: 04/22/2024 Cyl2 Install No.: 2

**Control Tests (0.100%)**

Installation Inlet: #2 (Lower) Post test active Cyl.: #1 (Upper)  
Dry Gas Lot No.: 302-402721128 Dry Gas Lot Exp.: 04/13/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	15:40:28		*TEST PASSED*
Control Test 1			1011	*TEST PASSED*
EC Result	0.097	15:41:17		*TEST PASSED*
IR Result	0.099	15:41:17		*TEST PASSED*
Ambient Air Blank	0.000	15:42:27		*TEST PASSED*
Control Test 2			1011	*TEST PASSED*
EC Result	0.097	15:42:54		*TEST PASSED*
IR Result	0.099	15:42:54		*TEST PASSED*
Ambient Air Blank	0.000	15:44:06		*TEST PASSED*
Control Test 3			1011	*TEST PASSED*
EC Result	0.097	15:44:34		*TEST PASSED*
IR Result	0.099	15:44:34		*TEST PASSED*
Ambient Air Blank	0.000	15:45:04		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Mimikos - First Name: Nicholas MI: E Badge No.: 7413

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*T.P.R.I. A.A. #7413*

Signed:

Date: 04/22/2024

ID: 3

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036  
DRAEGER MEDICAL SYSTEMS INC

Sales order: 1130435101  
Date: May 28, 2024

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-403035121  
ETHANOL IN NITROGEN

Manufactured Date: May 02, 2024  
Product Expiration: May 02, 2027

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	263.0	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND28529	103.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

#### TRACEABILITY

##### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1119668549  
Date: April 18, 2023

**DRAEGER MEDICAL SYSTEMS INC.;**

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402721128  
ETHANOL IN NITROGEN

Product Expiration: April 13, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	261.2	(0.100)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

#### TRACEABILITY

##### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.


Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: April 13, 2023

APPROVED BY: \_\_\_\_\_

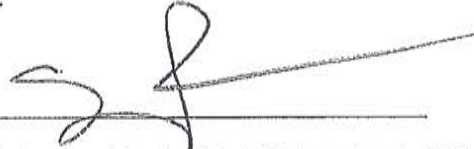

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251



  
**Dräger****Alcotest 9510****CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date: ✓

Serial Number:

6/6/2022ARMH-0009Dräger, Inc. GR



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 09/13/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1196 to 0.1212 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of September, 2023.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Customer: DRAEGER INC

7256 S SAM HOUSTON PKWY W

STE 100

HOUSTON, TX 77085

PO Number: S104303440829



## Certificate/SO Number: 5-F2R00-220-1 Revision 0

Manufacturer: Dräger Safety AG & Co. KGaA

Model Number: X-Cal 2000

Description: Breath Alcohol Simulator

Serial Number: ARRD-0003

ID: NONE

As-Found: In Tolerance

As-Left: In Tolerance

Issue Date: Oct 03, 2024

Calibration Date: Oct 03, 2024

Due Date: Oct 03, 2025

Calibrated To: Customer Specification

Calibration Procedure: 1-AC103519-1

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/INCSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/INCSL Z540.3-2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S104303440829



**Certificate/SO Number: 5-F2R00-220-1 Revision 0**

**As Found/As Left Data**

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	Cal Process		Measurement Uncertainty (k=2; ±)	Units	TUR
						O	T			
<b>Function Checks</b>										
Bubble Check			P	P	P					
Seal Check			P	P	P					
<b>Temperature Source: Accuracy Test</b>										
Accuracy Test	34.00°C	±( 0.02 °C)	33.98	34.02	34.01 °C		1.5e-002	1.6e-002	°C	1.3 : 1
<b>Temperature Source: Stability Test</b>										
Stability Test	0.00°C	±( 0.02 °C)	-0.02	0.02	0.00 °C		5.0e-003	7.6e-003	°C	4.0 : 1

Field not applicable.

**Traceable Standards**

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
05H1409	Mensor Corp	CPT9000	Precision Pressure Transducer	10-Jun-24	31-Dec-24	5-805H1409-3-1	AF/AL
HP927312	Hart Scientific/Fluke	1575	Super Thermometer	10-Jul-24	31-Jan-26	5-8HP927312-9-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

**Environmental Data**

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
70.00°F /21.11°C	54.00%	DewK8	G	Temperature

**Decision Rule**

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone

**CALIBRATED**  
BY **TRANSAT**

# CERTIFICATE OF CALIBRATION



**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S104303440829

**Certificate/SO Number: 5-F2R00-220-1 Revision 0**

are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S1O4303440829



Certificate/SO Number: 5-F2R00-220-1 Revision 0


### Legend

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

**CALIBRATED**  
BY **TRANSCAT**

# CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S1043034440829

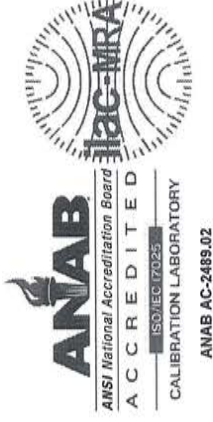

Certificate/SO Number: 5-F2R00-220-1 Revision 0

**Calibrated At:**  
16115 Park Row  
Houston, TX 77084

**Facility Responsible:**  
16115 Park Row  
Houston, TX 77084  
800-828-1470

**Unit Barcode:**  
  
09006587245


**Date Received:** October 01, 2024  
**Service Level:** R9

**Calibrated By:**  
  
Jose Martinez  
Calibration Technician  
Oct 03, 2024  
18:27:48 -04:00

**Reviewed By:**  
  
Daniel Beights for  
Lab Manager  
Oct 03, 2024  
19:24:44 -04:00

**Certificate - Page 5 of 5**  
Reprinted on October 18, 2024

**Customer Number:** 1-659111-000  
OPS-F20-014R11 07/27/23 FP001R9 4/9/2021

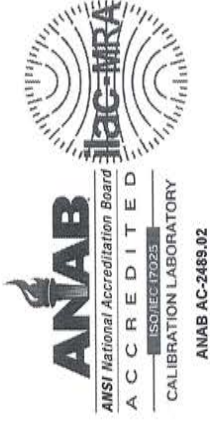

**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S1O4303405716

### Certificate/SO Number: 5-F2D8A-80-1 Revision 0

**Manufacturer:** Wilka Instr/Mensor Corp/Trend  
**Model Number:** CPG2300  
**Description:** Portable Barometer  
**Serial Number:** 41001RDG  
**ID:** NONE

**As-Found:** In Tolerance  
**As-Left:** In Tolerance  
**Issue Date:** Sep 27, 2024  
**Calibration Date:** Sep 26, 2024  
**Due Date:** Sep 26, 2025

**Calibrated To:** Manufacturer Specification  
**Calibration Procedure:** 1-AC94879-0

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/INCSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS 16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/INCSL Z540.3-2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.


Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances shown, these tolerances are either the original equipment manufacturers (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).



Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S104303405716

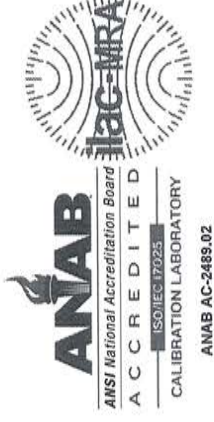

**Certificate/SO Number: 5-F2D8A-80-1 Revision 0**

**As Found/As Left Data**

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	O		Cal Process Uncertainty (k=2; ±)	Measurement Uncertainty (k=2; ±)	Units	TUR
						O	T				
<b>Pressure Measure: 8 to 17 psia Range</b>											
	7.985psia	±(0.015% FS)	7.982	7.988	7.983 psia			1.5e-004	6.0e-004	psia	19.8 : 1
	8.857psia	±(0.015% FS)	8.854	8.860	8.855 psia			1.7e-004	6.0e-004	psia	17.8 : 1
	9.731psia	±(0.015% FS)	9.728	9.734	9.730 psia			1.8e-004	6.0e-004	psia	16.2 : 1
	10.628psia	±(0.015% FS)	10.625	10.631	10.626 psia			2.0e-004	6.2e-004	psia	14.9 : 1
	11.647psia	±(0.015% FS)	11.644	11.650	11.646 psia			2.2e-004	6.2e-004	psia	13.6 : 1
	12.523psia	±(0.015% FS)	12.520	12.526	12.522 psia			2.4e-004	6.3e-004	psia	12.6 : 1
	13.396psia	±(0.015% FS)	13.393	13.399	13.394 psia			2.5e-004	6.3e-004	psia	11.8 : 1
	14.269psia	±(0.015% FS)	14.266	14.272	14.268 psia			2.7e-004	6.4e-004	psia	11.1 : 1
	15.270psia	±(0.015% FS)	15.267	15.273	15.268 psia			2.9e-004	6.4e-004	psia	10.3 : 1
	16.145psia	±(0.015% FS)	16.142	16.148	16.144 psia			3.1e-004	6.5e-004	psia	9.8 : 1
	17.020psia	±(0.015% FS)	17.017	17.023	17.018 psia			3.2e-004	6.6e-004	psia	9.3 : 1
	13.396psia	±(0.015% FS)	13.393	13.399	13.394 psia			2.5e-004	6.3e-004	psia	11.8 : 1
	12.523psia	±(0.015% FS)	12.520	12.526	12.522 psia			2.4e-004	6.3e-004	psia	12.6 : 1
	11.647psia	±(0.015% FS)	11.644	11.650	11.646 psia			2.2e-004	6.2e-004	psia	13.6 : 1

Field not applicable.

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S104303405716



**Certificate/SO Number: 5-F2D8A-80-1 Revision 0**

**Traceable Standards**

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
DW09BA	Fluke/DH Instruments	PG7601	Piston Gauge	11-Sep-23	30-Sep-24	5-&DW09BA-16-1	AF/AL
DW09CA	DH Instruments	MS-AMH-38	AMH Mass Set	13-Sep-24	13-Dec-24	5-&DW09CA-16-1	AF/AL
DW09LOW	Fluke/DH Instruments	PC-7100/7600-10-TC	Gas Piston-Cylinder Module	22-Aug-23	31-Aug-28	5-&DW09LOW-5-1	AF/AL
DW09MASS	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	1-Feb-24	30-Nov-24	5-&DW09MASS-9-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

**Environmental Data**

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
71.20°F /21.78°C	42.50%	DewK8	B	GP Pressure

**Decision Rule**

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S104303405716



Certificate/SO Number: 5-F2D8A-80-1 Revision 0

**Legend**

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

# CALIBRATED

BY **TRANSCAT**

# CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC

7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085

PO Number: S104303405716



Certificate/SO Number: 5-F2D8A-80-1 Revision 0

Calibrated At:  
16115 Park Row  
Houston, TX 77084

Facility Responsible:  
16115 Park Row  
Houston, TX 77084  
800-828-1470

Unit Barcode:   
0900B581617

Date Received: September 03, 2024  
Service Level: R9

Calibrated By:  
 Alex Spilker  
Alex Spilker  
Calibration Technician

Electronically Signed By:  
Alex Spilker

Sep 26, 2024 21:45:28 -04:00

Reviewed By:  
 Christopher Naylor for

Electronically Signed By:  
Christopher Naylor for

Sep 27, 2024 14:29:05 -04:00

Certificate - Page 5 of 5  
Reprinted on October 17, 2024

Customer Number: 1-659111-000  
OPS-F20-014R11 07/27/23 FP001R9 4/9/2021

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111663404

Date: July 05, 2022

**NJSP DEPT OF LAW AND PUBLIC SAFETY**

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402448282  
ETHANOL IN NITROGEN

Product Expiration: May 20, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>	<b>PPM</b>	<b>( BrAC )</b>
ETHANOL	263.3	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283190, 283189, 283188, or 283192 dated 6th January 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 20, 2022

APPROVED BY:

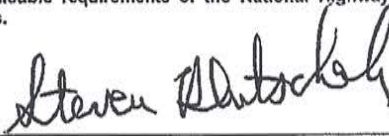

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111918174  
Date: July 27, 2022

**DRAEGER MEDICAL SYSTEMS INC.**

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402488140  
ETHANOL IN NITROGEN

Product Expiration: July 15, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	104.2PPM	(0.040)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	107.1	(0.041)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283192, dated 6th January 2022 or calibration test 292029, 292030 or 292031, dated 26th March 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: July 15, 2022

APPROVED BY: \_\_\_\_\_



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111713599

Date: July 05, 2022

NJSP DEPT OF LAW AND PUBLIC SAFETY

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402477282  
ETHANOL IN NITROGEN

Product Expiration: June 24, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	208.4PPM	(0.080)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	212.2	(0.081)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283190, 283189, 283188, or 283192 dated 6th January 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: June 24, 2022

APPROVED BY:

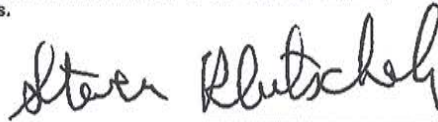

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111788955  
Date: July 14, 2022

NJSP

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402486005  
ETHANOL IN NITROGEN

Product Expiration: July 13, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	416.8PPM	(0.160)
NITROGEN	BAL	
<hr/>		
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	420.0	(0.161)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283192, dated 6th January 2022 or calibration test 292029, 292030 or 292031, dated 26th March 2022 applies

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: July 13, 2022

APPROVED BY: \_\_\_\_\_



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251



# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111709457  
Date: July 19, 2022

NJSP

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402488144  
ETHANOL IN NITROGEN

Product Expiration: July 15, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	781.5PPM	(0.300)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	785.3	(0.301)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283192, dated 6th January 2022 or calibration test 292029, 292030 or 292031, dated 26th March 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: July 15, 2022

APPROVED BY:





"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

DEPARTMENT OF  
*Water and Public Safety*  
 This is to certify that

**Nicholas E. Mimikos**  
**New Jersey State Police**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF  
 THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510  
 A METHOD TO DETERMINE INTOXICATION.  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One  
  
 COLONEL  
 NEW JERSEY STATE POLICE  
  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_



DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>7-14-23</u>	<u>Hamilton Tech</u>	<u>MF</u>
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 01/18)

DEPARTMENT OF  
*Water and Public Safety*  
 This is to certify that

**Nicholas E. Mimikos**  
**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF  
 THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510  
 A METHOD TO DETERMINE INTOXICATION.  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One  
  
 COLONEL  
 NEW JERSEY STATE POLICE  
  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 01/18)

DEPARTMENT OF  
*Motor and Public Safety*  
 This is to certify that

Robert W. Waldrop

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510  
 A METHOD TO DETERMINE INTOXICATION  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF March

TWO THOUSAND AND Twenty Four

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2936 (Rev. 10/22)

DEPARTMENT OF  
*Motor and Public Safety*  
 This is to certify that

Robert W. Waldrop

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510  
 A METHOD TO DETERMINE INTOXICATION  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF April

TWO THOUSAND AND Twenty Three

*[Signature]*  
 COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2936 (Rev. 10/22)