

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00864	Calib. Date:	05/04/2020
Certification File No.:	00865	Cert. Date:	05/04/2020
Linearity File No.:	00866	Lin. Date:	05/04/2020
Solution File No.:	00880	Soln. Date:	08/15/2020
Sequential File No.:	00880	File Date:	08/15/2020
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0164
Solution Control Lot:	19150	Expires:	06/10/2021
		Bottle No.:	0933

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:12D		
Control 1 EC	0.097%	20:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	20:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:13D		
Control 2 EC	0.096%	20:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	20:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:14D		
Control 3 EC	0.096%	20:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	20:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RUDITSKY

First Name: DAVID

MI: A

Signature: _____

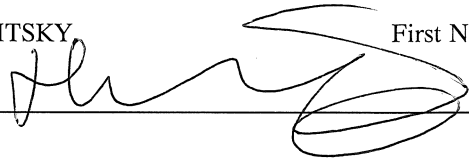

Badge No.: 090

Date: 08/15/2020

